


# I-JECT **B**uil **T** in **S**ystem

Digital Pain Free Automatic Syringe  
Digital Warmer & UV Sterilizer




# I-JECT Buil Tin System

## Dental Chair Built in no battery type pain-less automatic syringe

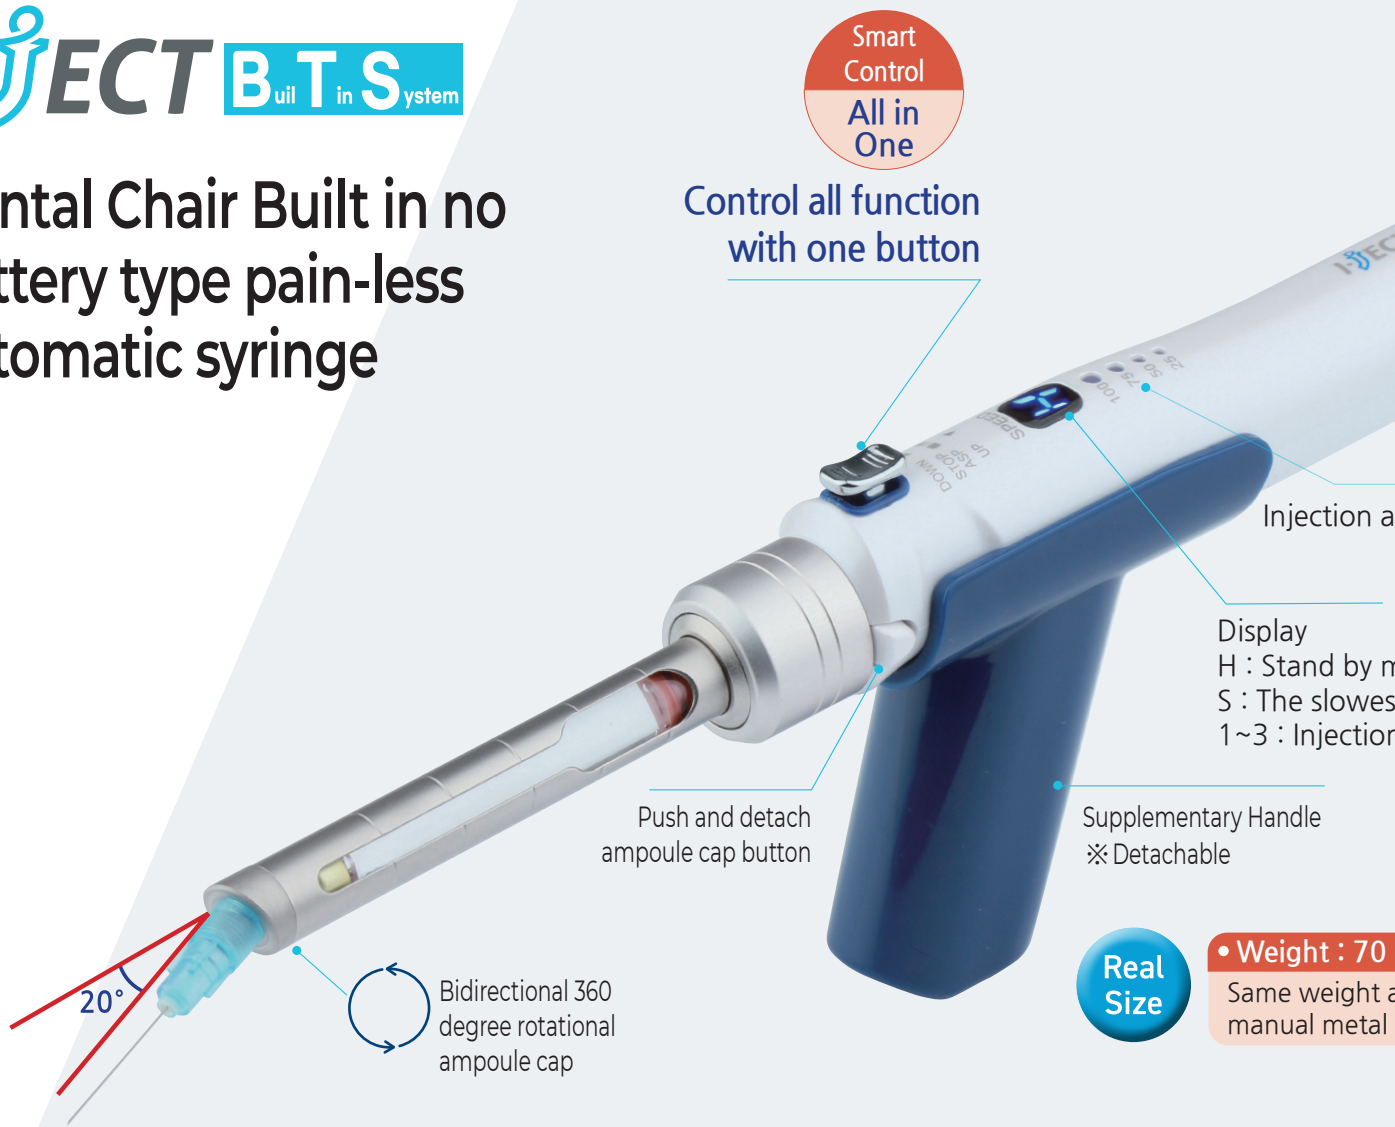


Implemented Auto Aspiration function for the first time in the world



### What was the most painful part of the anesthesia procedure?

52.7% of patients in the hospital reported the most severe was dental anesthesia.

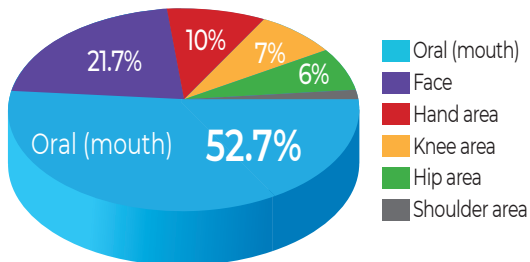

-Subject of survey : Consumer Survey on Hospital Anesthesia Injections  
 -Investigating Organization: Open survey panel  
 -Survey period : 2020. 03. 20 ~ 03. 20  
 -Respondents: total 300

### Offering two grip type

① Pen type



② Gun grip type (Attach)



### Example pictures of installment



# I-JECT B.T in S system

## Digital Warmer & UV Sterilizer

Offering optimal temperature to solve **Cold Pain!**

Turn On The New Warmth

Using dental chair power. Free from battery recharging.




Speaker

Voice notification

Promoting hospital or clinic ↑  
Offering relieve to patient

Mount LED



mode  
at injection  
n Speed

gram  
as  
syringe

n supplementary)



Manual syringe 2EA

Compatible with I-JECT ampoule cap and manual syringe.

Lidocaine ampoule 3EA



Manual syringe 2EA

Compatible with I-JECT ampoule cap and manual syringe.

Lidocaine ampoule 3EA

\* Devices on pictures are not included except transparent tray.



▲ Preventing contamination by UV sterilization of needle insert point

Speaker

Voice notification


- Start sterilization (When closing the cover)
- Sterilization is complete (Sterilization Completion time : 3 minutes)

OPTION



I-JECT B.T in S

MEDIHUB



medihub2

Front view

Side view

Internal UV sterilization function




Proved COVID-19 virus sterilization!

NEW

Brand new contra ampoule cap can raise success rate of nerve block anesthesia.



Maximized comfortable dental anesthesia treatment



- ☑ Comfortable anesthesia on block, low and upper jaw posterior region
  - ☑ Free from bended needle broken
  - ☑ 360° bidirectional rotation
- ◀ Example of clinical use



Inquiry ☎ + 82 70 4250 3990

Head (15808) #108, 201 SA Tower, 175. LS-ro, Gunpo-si  
Office Gyeonggi-do, Republic of Korea

T. + 82-70-7711-2007 / F. + 82 505 365 6126

Email : medihub@medihub.co.kr

Website : www.medihub.co.kr  
www.iject.kr

### Pain Control Package

NEW

I-JECTION



Digital Warmer & UV Sterilizer

i-JECT



Digital Pain Free Automatic Syringe